



LINK Embrace

Reverse Primary Shoulder Technique

Explanation of Pictograms			
	Manufacturer		Article number
	Material (number)	Rx only	Caution: Federal law restricts this device to sale by or on the order of a physician

LINK Embrace

Shoulder System Reverse Configuration

Chapter	Surgical Technique:	
1.	Pre-Op Planning	02
2.	Surgical Approaches and Patient Positioning	02
3.	Color Coding	03
4.	Humeral Resection and Preparation	05
5.	Reverse Glenoid Preparation and Implantation	16
6.	Reverse Humeral Component Trialing and Implantation	28
7.	Component Removal	36
8.	Implants	41
9.	Instruments	49
10.	Accessories: X-ray Templates	55
11.	System Compatibility	55
	Important Information	

1. Pre-Op Planning

The operation is planned with the assistance of standard X-rays with normal AP-view in internal and external rotation as well as an axillary view. For implantation of a glenoid component and in fracture cases a CT scan is recommended to better assess the glenoid configuration. Additionally, MRI may be indicated for assessment of the degree of bone deficiency as well as soft tissue and capsule quality. Neurological exams should be performed in post-traumatic and disabling shoulder cases.

LINK Embrace X-ray templates are available for pre-op planning of osteoarthritic cases, and they may also be used in fracture and revision cases as far as applicable. LINK Embrace X-ray templates have a 105% scale. Several digital planning platforms are supported.

2. Surgical Approaches and Patient Positioning

2.1 Surgical Approaches

The LINK Embrace Shoulder System is suitable for implantation using the existing surgical approaches. The instrument set supports the two most popular surgical approaches to the shoulder joint, delto-pectoral and lateral approach. Usually, the selected approach depends on the surgeon's experience and preferences, furthermore, the diagnosis and planned surgical treatment have to be taken into account. With the patient under anesthesia, glenohumeral ROM is evaluated in order to assess the extent of capsular release needed to restore the ROM postoperatively.

2.2 Patient Positioning

It is recommended to perform shoulder arthroplasty in a beach-chair position. This allows for full access to the shoulder joint which is necessary to intraoperatively assess the joint function, stability and range of motion. To facilitate access to the joint and, if required, the use of fluoroscopy, the patient should be positioned as lateral as possible to the affected side on the OR table. The head needs to be securely fixed.



Figure 2.1

3. Color Coding

The LINK Embrace Shoulder System offers diverse fixation and biomechanical options. The options offered by each implant are indicated by a color-coding matrix on each component package. Color-coding matrix 1 (figure 3.1) is applied on all implant components except Bone Screws, for which color-coding matrix 2 is used (figure 3.2). Matrix 1 (figure 3.1) consists of seven cells in total. The first line contains product related information, such as component size, length or assignment. The left column indicates the possible biomechanical configurations the component can be used for. The right column indicates the fixation options to anchor the implant in the bone. The meaning of each cell is explained in table 3.1 below. Available options are highlighted by a specific color, and options not available are indicated by a grey cell (figure 3.2, right matrix).

L 100	Ø 13
Anatomical	Cementless
Reverse	Cemented
CTA	Hybrid

Figure 3.1 Example Color Coding Matrix 1

Color-coding matrix 2 (Figure 3.2) consists of four cells in total. The left column indicates the possible biomechanical configurations the component can be used for. The meaning of each cell is explained in table 3.1. Available options are highlighted by a specific color, options not available are indicated by a grey cell (figure 3.2, right matrix). The central cell contains the screw length L (in mm) in the first line and the screw diameter (in mm) in the second line. The right cell indicates the screw type according to the three symbols explained in table 3.1.

Anatomical	L20	
Reverse	Ø 6.0	

	L20	
Reverse	Ø 6.0	

Figure 3.2 Example Color Coding Matrix 2



Anatomical	Indicates the component can be used for anatomical configurations (TSA). Please note this code also applies to Hemi Shoulder Arthroplasty (HEMI) when the glenoid is left native.
Reverse	Indicates the component can be used for reverse configurations (RSA).
CTA	Indicates the component is a CTA head or can be combined with a CTA head.
Cementless	Indicates cementless component fixation in the bone.
Cemented	Indicates cemented component fixation in the bone.
Hybrid	Indicates simultaneous cemented and cementless component fixation in the bone. Please refer to the surgical technique for further information.
	Indicates a central Bone Screw to be applied with the Convertible Metal-Back or Reverse Glenoid Baseplate.
	Indicates a peripheral angle-stable Bone Screw to be applied with the Reverse Glenoid Baseplate.
	Indicates a peripheral non angle-stable Bone Screw to be applied with the Reverse Glenoid Baseplate.

Table 3.1

4. Humeral Resection, Preparation

This chapter describes the surgical technique for reverse Total Shoulder Arthroplasty using

- Humeral Standard Stems and Humeral Short Stems
- Reverse Trays and Reverse Inserts
- Reverse Glenoid Baseplates and Glenospheres

The LINK Embrace Shoulder System offers components for both primary and revision surgery applying to reverse joint configurations.

A multi-option Reverse Glenoid Baseplate, available with standard and long peg for revisions, hosts the Glenospheres. Several options, e.g. inclined Reverse Trays and Inserts, allow for individual adaption of the joint kinematics to the patient requirements.

4.1 Humeral Head Resection

4.1.1 Intramedullary Alignment



Figure 4.1

Expose and mobilize the humeral head and luxate it from the glenoid.



Figure 4.2

Open the medullary canal with a suitable instrument in line with the humeral axis.

Using the T-Handle, insert the Starter Awl into the medullary canal until the depth stop is reached. Make sure that the blue Depth Stop Disk rests in the Starter Awl shaft recess.



Figure 4.3

Prepare the Resection Guide depending on the surgical approach, i.e. selection of the Resection Block for delto-pectoral or for lateral approach.

NOTE: The LINK Embrace Instrument Set supports different surgical approaches. In the surgical technique described here, the delto-pectoral approach is used.

For lateral techniques use the Resection Block for lateral approaches and follow the workflow correspondingly.



Figure 4.4

Slide the Resection Guide down on the Starter Awl placed in the medullary canal by applying light pressure to the instrument spring clamp.



Figure 4.5

Connect the desired Resection Block and the Resection Guide Connector with the laser marks on both Connector Bar and Resection Block in line. The Resection Block is fixed to the Connector Bar by means of a magnetic connection.



Figure 4.6

Considering the side to be treated, insert the Resection Guide Connector into the fork of the Resection Guide. A slight initial resistance prevents the instrument from slipping out of the fork.



Figure 4.7

According to the desired retroversion, screw the Alignment Rod into the corresponding hole (0°, 10°, 20°, 30°) in the Alignment Rod Connector. Make sure to select the correct set of holes for treatment of the left or right side respectively, corresponding to the laser marking on the Alignment Rod Connector.



Figure 4.8

Place the Alignment Rod Connector in the required orientation (Left or Right) on the Resection Guide.



Figure 4.9

Set the desired retroversion by axially rotating the Resection Guide on the Starter Awl, adjusting the Alignment Rod parallel to the forearm which is held flexed at approx. 90°.

Adjust the Resection Guide to the desired resection level (to change the instrument level, press the instrument spring). The spring locks the instrument when released.

Finally determine the resection level with respect to the anatomical neck of the humeral head.

Slide the Resection Block together with the Resection Guide Connector within the fork until it makes contact with the bone.

Fix the Resection Block with at least two Fixation Pins (3.0 mm) using the Universal Pin Inserter.



Figure 4.10



Figure 4.11

The medial and lateral pin axis are parallel to each other and will allow sliding of the resection block. The central pin axis is oblique and will fix the block in place.

The orientation of the pinholes is marked accordingly on the block. Take note that the most lateral pin might interfere with the intramedullary Starter Awl.



After a final check of the resection level and retroversion, the humeral head is resected with an oscillating saw blade on top of the Resection Block at 135° (defined by the instrument).

For this purpose, all instruments except the fixed Resection Block can be removed by pulling them upwards. To do so, press the spring on the Resection Guide, and slide the Resection Guide upwards over the Starter Awl. Then remove the Starter Awl using the T-Handle.



Figure 4.12

For more stability, e.g. in case of poor fixation, the Resection Guide can also be left in place. When sawing, make sure to avoid any instrument interference.



Figure 4.13

Remove all instruments. Pins can be removed with the Pin Inserter/Extractor.

4.1.2 Extramedullary Alignment



Figure 4.14

Alternatively to intramedullary alignment, use the Resection Guide for extramedullary alignment. The extramedullary Resection Guide has a built-in angle of 135°.



Figure 4.15

According to the desired retroversion, screw the threaded end of the Alignment Rod into the corresponding hole (0°, 10°, 20°, 30°) on the vertical Resection Guide bar. The guide has two opposing sets of holes for left and right application.



Figure 4.16

Align the rod-shaped neck of the instrument along the humeral shaft axis. A second Alignment Rod may be screwed into the hole at the distal guide end, prolonging the instrument axis for easier positioning.



Figure 4.17

Set the desired retroversion by internal or external rotation of the Guide, adjusting the Alignment Rod parallel to the forearm which is held flexed at approx. 90°.



Figure 4.18

Determine the final resection level with respect to the anatomical neck of the humeral head. Fix the Resection Guide with at least two Fixation Pins (3.0 mm) using the Universal Pin Inserter. The medial and lateral pin axis are parallel to each other and will allow sliding of the resection block. The central pin axis is oblique and will fix the block in place.

The orientation of the pinholes is marked accordingly on the block.

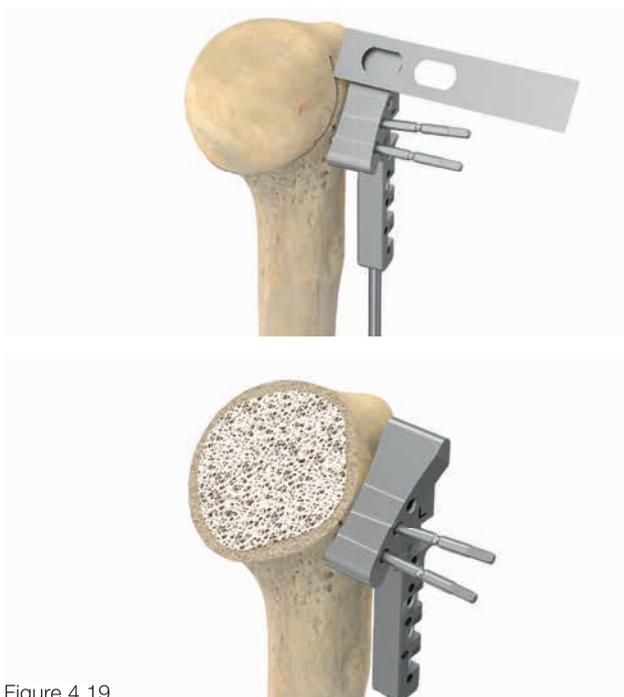


Figure 4.19

After a final check of level and retroversion, resect the humeral head with an oscillating saw blade on top of the Resection Guide.

4.1.2.1 Alternative Retroversion Determination



Figure 4.20

The LINK Embrace Instrument Set supports an alternative way to determine the retroversion, using the Alignment Rod and the Alignment Rod Connector.



Figure 4.21

Place the Alignment Rod Connector with the Alignment Rod in the required orientation on the Resection Guide.

Go on as described in 4.1.2

4.2 Humeral Standard and Short Stem Preparation

NOTE: The LINK Embrace System offers Humeral Stems in two different lengths: Humeral Standard Stems of 100 mm and Humeral Short Stems with 75 mm length. Dedicated Humeral Compressors are used for both ranges. The Compressors are 5 mm longer than the corresponding Stems.



Figure 4.22

Medullary canal preparation is started with the smallest Compressor (size 12) in the required length (75 mm or 100 mm).

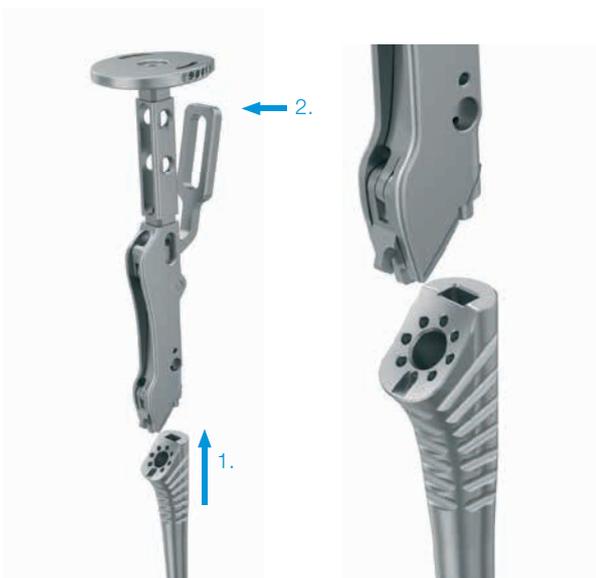


Figure 4.23

Connect the Compressor to the Handle for Compressors and Proximal Bodies by opening the lever and inserting the nose piece at the end of the Handle into the Compressor's groove located laterally. Close the lever, locking the Compressor firmly to the Handle.



Figure 4.24

According to the desired retroversion, screw the threaded end of the Alignment Rod into the corresponding hole (0°, 10°, 20°, 30°) in the rim of the Handle impactation plate. Make sure to select the correct set of holes for treatment of the left or right side respectively.



Figure 4.25

Alternatively, the Alignment Rod may be used together with the Alignment Rod Connector to determine the desired retroversion as described in 4.1.1.

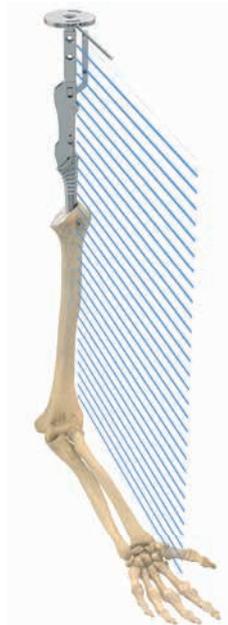


Figure 4.26

Insert the Handle with the Compressor into the humeral shaft. Set the desired retroversion by axially rotating the Handle, adjusting the Alignment Rod parallel to the forearm which is held flexed at approx. 90°.



Figure 4.27

Gradually prepare the humeral canal until the size determined in the preoperative planning is reached. The Compressor has to be stable and the line mark on the Handle has to be flush with the resection surface (red circle). The Compressor is now slightly recessed within the bone.



Figure 4.28

Remove the Handle, leaving the last Compressor in situ. Connect the Finishing Reamer with the T-Handle (Hudson fitting).



Figure 4.29

Ream the humeral resection surface with the Finishing Reamer and create a concave front face. To do so, insert the blue Reamer guide tip into the female taper of the humeral Compressor and align axially.



Figure 4.30

Ream manually until the depth stop is reached. Remove the Reamer.



Figure 4.31

Depending on the posterior head offset, choose the appropriate Humerus Protection Plate from two options: neutral or 6 mm offset version.

Place the selected Humerus Protection Plate on the resection surface with its peg in the central hole of the humeral component.

Depending on the preferred workflow, glenoid preparation can be performed immediately after humeral head resection. The Humerus Protection Plates can also be placed directly onto the bone and be fixed with the aid of the backside pins.

Go on with chapter 5.

5 Reverse Glenoid Preparation and Implantation

5.1 Glenoid Positioning



Figure 5.1

Sublux the humerus posterior-caudally with the help of a double fork retractor or a Fukuda retractor. Excise labrum and osteophytes to expose the glenoid. Connect the K-Wire Positioner for Reverse Baseplate to the Handle for Glenoid Sizers and Drill Templates (magnetic connection).



Figure 5.2

Place the K-Wire Positioner according to your preferences. Usually, the Positioner is placed as inferiorly as possible, avoiding any overhang of the Positioner with respect to the bony glenoid rim. Place the K-Wire for Glenoid Preparation (max. Ø 2.5 mm) with the drilling machine through the central hole of the Positioner in the desired direction.



Figure 5.3

After removal of the Positioner, visually check the correct position of the K-Wire and reposition it if necessary. To do so, use the Repositioner for K-Wires. The Repositioner for K-Wires allows for parallel shifting the K-Wire in 3, 4 and 7 mm distance. Depending on the required offset, slide the Repositioner over the K-Wire through the corresponding hole down to the glenoid and align the offset.



Figure 5.4

Insert a second K-Wire through the specified lumen. After removal of the Repositioner, visually check the correct position of the K-Wire. Remove the initially positioned K-Wire with the Pin Inserter/Extractor.



Figure 5.5

NOTE: Alternatively, the K-Wire may be placed through the cannulated Guide Handle for K-Wire, ensuring perpendicular alignment of the K-Wire with respect to the K-Wire Positioner.



Figure 5.6

To do so, place the Guide Handle for K-Wire on the Positioner so that the two Guide noses click into the grooves of the Positioner (magnetic connection).



Figure 5.7

Place the instrument on the glenoid according to your preferences. Usually, the Positioner is placed as inferiorly as possible, avoiding any overhang of the Positioner with respect to the bony glenoid rim. Place a K-Wire through the Guide Handle into the glenoid bone.

5.2 Glenoid Reaming



Figure 5.8

Glenoid reaming is carried out with the Glenoid Reamer size S (Ø 28 mm).

NOTE: LINK Embrace Glenoid Reamers have a slotted central hole, allowing for slightly tilting the Reamer on the K-Wire. A cut-out at the outer Reamer ring facilitates passing the surrounding soft tissue and, thus, pushing the Reamer down to the glenoid.

Select the Glenoid Reamer of size small (Ø 28 mm), tilt it and slide over the K-Wire down to the glenoid.



Figure 5.9

Slide the cannulated Drive Shaft for glenoid preparation (with the Tissue Protection Sleeve installed) over the K-Wire and insert it into the situs. Connect the Drive Shaft to the Glenoid Reamer in situ. To do so, insert the external hexagon of the Drive Shaft into the internal hexagon of the Reamer (magnetic connection).

Carefully ream the glenoid. For manual reaming, connect the T-Handle to the Drive Shaft employing the Hudson fitting.



Figure 5.10

NOTE: Take into account the stability of the bone. Avoid applying excessive forces and overreaming of the glenoid. It is recommended to carefully place the reamer onto the glenoid. When using a power tool, have it already rotating before contact.

After reaming, remove the Drive Shaft and Reamer in reverse order, leaving the K-Wire in situ.

5.3 Drilling of Central Hole for Reverse Glenoid Baseplates

NOTE: LINK Embrace Reverse Glenoid Baseplates are available with standard peg (15 mm) and long peg (25 mm). Depending on the required peg length, select the appropriate Drill for the central peg hole.



Figure 5.11

Drill the central hole for the central peg of the Reverse Glenoid Baseplate with the Drill for Central Pegs of Reverse Glenoid Baseplate over the K-Wire. To do this, attach the corresponding Drill (standard or long) for Central Pegs to the Drive Shaft (hexagon with magnetic connection) and drill until the depth stop is reached.

Remove all instruments.

5.4 Reverse Glenoid Baseplate Implantation



Figure 5.12

Slide the threaded Shaft for Impactor into the Impactor. Turn it clockwise to pass the safety thread that prevents the Shaft from slipping out of the Impactor.



Figure 5.13

Attach the required Reverse Glenoid Baseplate to the Impactor and fix it by turning the inner Shaft clockwise using the Torx 20 Screwdriverbit connected to the Ratchet. When connecting the Reverse Baseplate to the Impactor, align the “S/I” (superior/inferior) laser mark on the Impactor with the “S/I” mark on the Reverse Baseplate rim.



Figure 5.14

With the Reverse Glenoid Baseplate firmly fixed to the Impactor, the instrument is introduced into the situs. Prior to impaction make sure that the “S/I” mark on the Reverse Glenoid Baseplate rim is oriented superiorly. Usually, the superior hole is directed towards the coracoid base. With the component aligned in the described way, axially impact the Baseplate until it is fully seated.

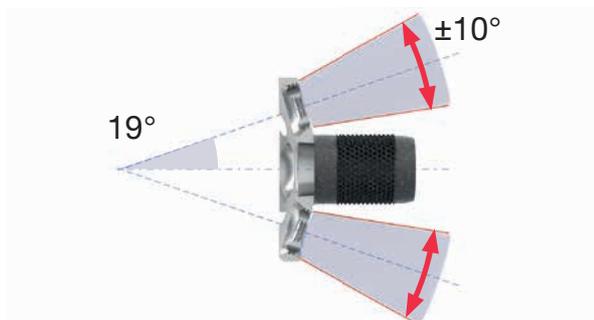


Figure 5.15

NOTE: LINK Embrace Reverse Glenoid Baseplates anchor in the bone using a central pressfit peg and up to four peripheral Bone Screws. If required, a central Bone Screw can be applied through the central peg for additional fixation. Peripheral Screws are available as Ø 6.0 mm cancellous Bone Screws, Ø 4.5 mm cortical Bone Screws and Ø 4.5 mm angle-stable cortical Bone Screws.

All peripheral screw holes of the Reverse Glenoid Baseplate can be filled with any of these screw types. It should be noted that the superior and inferior screw holes allow for polyaxial alignment of angle-stable (locking) screws, in which the screw angle can be selected within a range of $\pm 10^\circ$ from the neutral position. The neutral position of the superior and inferior holes is designed 19° divergent in relation to the central peg. Likewise, the posterior and anterior screw holes allow for monoaxial alignment of angle-stable (locking) screws. The axes of the posterior and anterior screw holes are designed monoaxial and parallel to the central peg.

All peripheral Bone Screws are available in lengths 20, 25, 30, 35, 40, 50 and 60 mm and have a self-tapping tip. They are tightened using the Torx 25 Screwdriverbit connected to the Ratchet.

5.4.1 Reverse Glenoid Baseplate: Use of Central Bone Screws

NOTE: If required, LINK Embrace Reverse Glenoid Baseplates can additionally be fixed with a central Bone Screw. For this purpose, 6.0 cancellous central screws are available in lengths of 20 mm, 25 mm and 30 mm.



Figure 5.16

Insert the Drill Guide for central Screws into the Reverse Glenoid Baseplate central hole. The Drill Guide determines the direction of the screw. Drill the screw hole with the Ø 3.2 mm Drill to the desired depth.



Figure 5.17

The required screw length is determined with the Depth Gauge.



Figure 5.18

The cancellous cylinder head Screw of the desired length is inserted with the Torx 25 Screwdriverbit, which is connected to the Ratchet and tightened until it is fully seated.

NOTE: Make sure the Bone Screw is fully seated. Go on tightening the Bone Screw until the laser mark on the Screwdriverbit is level with the Reverse Baseplate surface, indicating the Bone Screw is in the required position.

NOTE: Care must be taken to not overtighten the central Bone Screw as this might impair the fixation of the Screw or damage the bone.

5.4.2 Superior and Inferior Bone Screws (angle-stable and non angle-stable)



Figure 5.19

Insert the “S/I” polyaxial Drill Guide with its rear peg into the central Baseplate hole. The small outrigger will only allow the Drill Guide to mate to the Baseplate in the correct axis. The Drill Guide should sit firmly on the Baseplate.

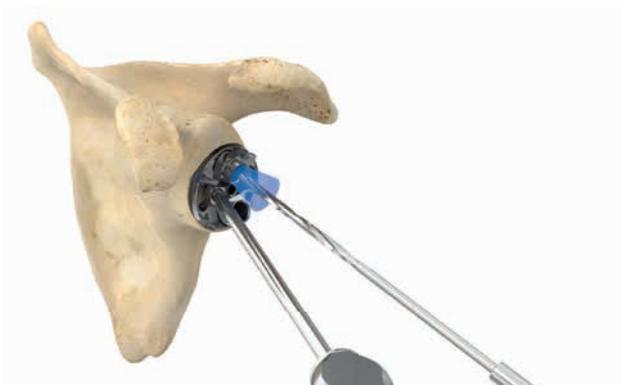


Figure 5.20

The Drill Guide limits the possible angulation range of the drill. Make sure to not exceed this under any circumstances.



Figure 5.21

Select an appropriate angle and drill the screw hole with the Ø 3.2 mm drill to the desired depth. Usually, the superior screw is directed towards the coracoid base. Determine the required screw length with the Depth Gauge.



Figure 5.22

Select the required screw type from Ø 6.0 mm cancellous Bone Screws, Ø 4.5 mm cortical Bone Screws or Ø 4.5 mm angle-stable (locking) cortical Bone Screws.

NOTE: in case the use of both angle-stable (locking) and standard (non angle-stable) Bone Screws is intended, it is recommended to apply the standard screws first in order to achieve compression between Baseplate and glenoid bone.

Insert the selected Bone Screw with the Torx 25 Screwdriverbit connected to the Ratchet and tighten the Screw until it is fully seated.

NOTE: Make sure the Bone Screw is fully seated in order to avoid mechanical contact between Glenosphere backside and Bone Screw head.

Apply the same procedure for the inferior Bone Screw.

5.4.3 Posterior and Anterior Bone Screws



Figure 5.23

Insert the A/P monoaxial Drill Guide into the posterior screw hole. The Drill Guide determines the direction of the screw. Drill the screw hole with the Ø 3.2 mm Drill to the desired depth.

The required screw length is determined with the Depth Gauge. Select the required screw type from Ø 6.0 mm cancellous Bone Screws, Ø 4.5 mm cortical Bone Screws or Ø 4.5 mm angle-stable cortical Bone Screws. Insert the selected Bone Screw with the Torx 25 Screwdriverbit, which is connected to the Ratchet, and tighten it until it is fully seated.

NOTE: Make sure the Bone Screw is fully seated in order to avoid mechanical contact between Glenosphere backside and Bone Screw head.

Apply the same procedure for the anterior screw.



Figure 5.24

5.5 Glenospheres

NOTE: LINK Embrace Glenospheres made of EndoDur are available in 36 mm, 39 mm and 42 mm diameters in both neutral (concentric) and eccentric versions. They are to be combined with Reverse Inserts made of UHMWPE with the same diameter. All Glenospheres are fixed in the Reverse Glenoid Baseplate with a taper connection and a pre-assembled locking screw.

All LINK Embrace Glenospheres have an overhang of the dome which has to be placed inferiorly.



Figure 5.25

5.5.1 Trial Glenospheres

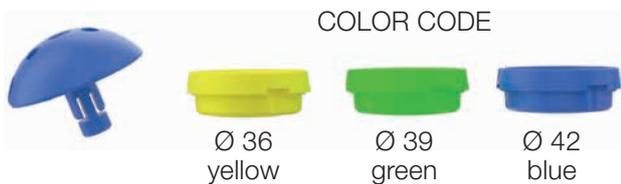


Figure 5.26

After implantation of the Reverse Glenoid Baseplate and appropriate preparation of the humeral component, a trial reduction may be performed using the neutral (concentric) or eccentric Trial Glenospheres of the required diameter. The sizes of the Trial Glenospheres and Reverse Trial Inserts are color coded:

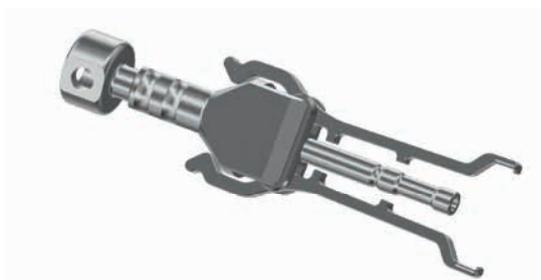


Figure 5.27

The required Trial Glenosphere is placed on the Reverse Glenoid Baseplate by means of the Handle for Glenospheres.



Figure 5.28

To do so, turn the knob of the instrument counter-clockwise to open the pincers. According to the type of Glenosphere used, select the Cap for neutral (short) or the Cap for eccentric Glenospheres (long) respectively and slide it on the central Handle rod between the pincers. When using the Cap for eccentric Glenospheres make sure the Cap is aligned with the recessing side of the tip inferiorly.

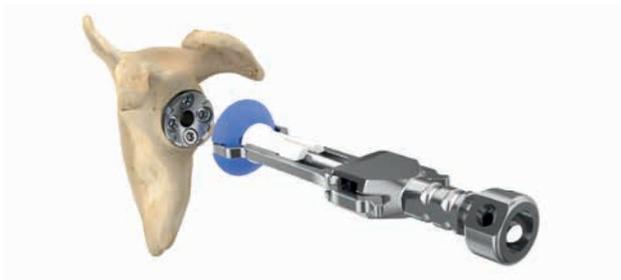


Figure 5.29

Place the required Trial Glenosphere in the Handle with the pincers positioned in the lateral grooves of the Glenosphere. Make sure the Handle and Glenosphere are axially aligned and the Cap is flush with the Glenosphere. Turn the instrument knob clockwise to close the pincers and to fix the Trial Glenosphere.



Figure 5.30

With the Handle, insert the Trial Glenosphere and press it firmly into the Reverse Baseplate to engage the taper connection.



Figure 5.31

Make sure the Trial Glenosphere does not interfere with bone or soft tissue, in particular on the superior edge. In case of contact to bone or other tissue, remove the component and excise the bone or tissue in the area of contact. Then reintroduce the Trial Glenosphere.

Remove the Handle for Glenospheres by turning the knob counterclockwise.

With the humeral trial component completely prepared, perform a trial reduction.

5.5.2 Glenospheres: Implantation

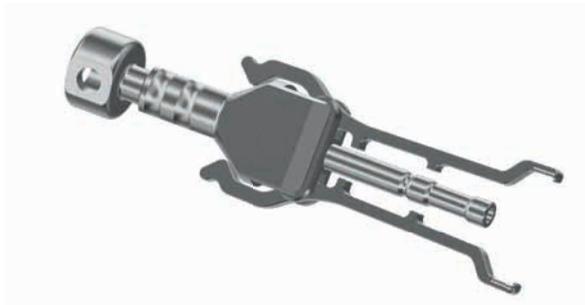


Figure 5.32

If used, remove the Trial Glenosphere. The required Glenosphere is placed on the Reverse Glenoid Base-plate by means of the Handle for Glenospheres.



Figure 5.33

To do so, turn the instrument knob counterclockwise to open the pincers. According to the type of Glenosphere used, select the Cap for neutral (short cap) or the Cap for eccentric Glenospheres (long cap) respectively and slide it on the central Handle rod between the pincers. When using the Cap for eccentric Glenospheres make sure the Cap is aligned with the recessing part of the tip inferiorly.



Figure 5.34

Place the required Glenosphere in the Handle with the pincers positioned in the lateral grooves of the Glenosphere. Make sure Handle and Glenosphere are axially aligned and the Cap is flush with the Glenosphere. Turn the instrument knob clockwise to close the branches and fix the Glenosphere.



Figure 5.35

NOTE: If a central Bone Screw is implanted, recheck the full seating of the Screw prior to Glenosphere insertion in order to avoid any contact between Bone Screw head and Glenosphere fixation screw.

Insert the Glenosphere into the Reverse Baseplate. Make sure the component overhang is positioned inferiorly and the taper engages with the inner taper of the Reverse Baseplate. Make sure the Glenosphere does not interfere with bone or soft tissue, in particular at the superior edge. In case of contact to bone or other tissue, remove the component and excise the bone or tissue in the area of contact. Then reintroduce the Glenosphere. Carefully impact the Glenosphere with slight mallet blows onto the Handle impaction plate to engage the taper connection.



Figure 5.36

Check the seating of the taper connection by gently applying rotational forces with the Handle. The taper is engaged when the Glenosphere resists against axial and rotational forces.

Connect the Torx 20 Screwdriverbit to the 3 Nm Torque Wrench. Slide the assembled Screwdriver through the Handle for Glenospheres. Tighten the internal fixation screw by turning the 3 Nm Torque Wrench clockwise. The required torque of 3 Nm is reached when a clicking noise can be heard.



Figure 5.37

Remove the Torque Wrench and the Handle for Glenospheres by turning the Handle knob counterclockwise.

With the humeral components/trial components completely prepared, perform a trial reduction.

6 Reverse Humeral Component Trialing and Implantation

NOTE: The LINK Embrace System offers three different Reverse Trays and Trials to accommodate Reverse Inserts. Reverse Trays are mounted onto the humeral components (Compressors, Humeral Standard and Short Stems). Reverse Trays come in neutral (concentric), 10° inclined and 3 mm offset versions.



Figure 6.1



Figure 6.2

Reverse Trial Trays in inclined and offset versions as well as the respective final Reverse Trays can be rotated in 45° steps to individually adjust various parameters such as inclination, retroversion, (posterior) offset and humerus lateralization. A scale on the Tray front side is used to determine the orientation of both the Reverse Tray and the Reverse Insert. It helps with later reproduction of the selected trial configuration with the final prosthesis components. It is recommended to start trialing with a neutral Reverse Tray.



Figure 6.3

LINK Embrace Reverse Inserts are available in different diameters, heights and inclinations according to table 6.1. They have to be combined with LINK Embrace Glenospheres of the same diameter.

Reverse Humeral Inserts		
Diameter Ø	Inclination	Heights
		UHMWPE
36	0°	0, 3, 6
	10°	0, 3, 6
	20°	0, 3, 6
39	0°	0, 3, 6
	10°	0, 3, 6
	20°	0, 3, 6
42	0°	0, 3, 6
	10°	0, 3, 6
	20°	0, 3, 6
to be combined with Glenospheres made of:		EndoDur

Table 6.1: Reverse Inserts: types and allowed combinations. Numerical data in mm unless otherwise noted.



Figure 6.4

All LINK Embrace Reverse Inserts can be fixed in any position on the Reverse Trays. In combination with a Reverse Tray, different parameters such as inclination and retroversion can be adjusted independently in the respective spatial planes.

Both the inclined trial and the inclined final Reverse Inserts have a line mark that indicates the highest point, which is used to determine the orientation of the Reverse Trial Insert. It helps with later reproduction of the selected trial configuration with the final prosthesis components.

It is recommended to start trialing with a neutral Reverse Insert with height 0.

6.1 Humeral Standard and Short Stem Trialing



Figure 6.5

Place the neutral Reverse Trial Tray on the humeral component and press it down firmly until it is fully seated. A spring-loaded clamp connection fixes the Trial Tray to the humeral component.



Figure 6.6

Select the suitable Reverse Trial Insert (diameter and height).

NOTE: The LINK Embrace System includes Reverse Inserts and trial components in various diameters, inclinations and heights. It is recommended to start with a neutral (0° inclination) Reverse Trial Insert with 0 mm height.

Using the Insertion Forceps, place the Reverse Trial Insert in the Reverse Trial Tray.



Figure 6.7

Perform a trial reduction to check stability, tension and function of the joint.

NOTE: If required, the joint configuration may be adapted by selecting a Reverse Trial Tray with offset or inclination and/or Reverse Trial Inserts with different height and/or inclination. Reverse Trial Trays and final Reverse Trays have a dial-like ring on their front side used to precisely determine and reproduce the selected position. For this purpose, the most laterally located digit on the Trial is noted and the final Reverse Tray is later on positioned accordingly with the same digit most laterally. In case an inclined Reverse Insert is used, the position of the mark indicating the highest point is noted as well.



Figure 6.8

Go on with chapter 6.3.1.

6.2 Humeral Components: Implantation

6.2.1 Humeral Standard and Short Stem Implantation

6.2.1.1 Cementless Humeral Standard and Short Stem Implantation

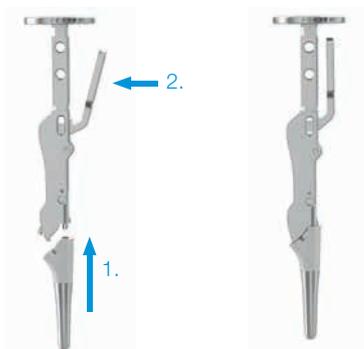


Figure 6.9

NOTE: For cementless implantation, the Humeral Standard or Short Stem of the same size as the last Compressor is used. Compressors and Stems with the same size designation have identical dimensions (Compressors have + 5 mm length).

Remove the transportation lock (white plastic cover) from the selected Humeral Stem. Connect the Humeral Stem to the Handle.



Figure 6.10

Impact the Humeral Stem taking into account the desired retroversion. For this purpose, the Alignment Rod is screwed into the appropriate hole in the Handle impactation plate rim. Make sure to select the correct set of holes for left and right side treatment.



Figure 6.11

Alternatively, place the Alignment Rod Connector on the Handle and insert the Alignment Rod in the appropriate hole. Make sure to select the correct position of the Alignment Rod Connector for left and right side treatment.



Figure 6.12

At first, the Humeral Stem should not be completely impacted but protrude slightly from the humerus. This facilitates the complete coupling of the taper connection between Humeral Stem and Reverse Tray.

Place the required Reverse Tray, reproducing the configuration selected in the trial reduction. For offset and inclined Reverse Trays, the same digit as the digit determined with the trial prosthesis must be aligned laterally.



Figure 6.13

Insert the Fixation Screw into the Reverse Tray (supplied with the Reverse Tray).



Figure 6.14

Connect the Torx 25 Screwdriverbit to the 3 Nm Torque Wrench.



Figure 6.15

Position the tips of an appropriate instrument, e.g. a LINK Bankart Perforating Forceps (item code 64-4160/09) into the grooves of the Reverse Tray and hold the instrument firmly.



Figure 6.16

Introduce the prepared Screwdriver into the Fixation Screw within the Reverse Tray. Tighten the Screw by turning the Screwdriver clockwise while holding the Forceps firmly in place with your other hand. The required torque of 3 Nm is reached when a clicking noise can be heard.



Figure 6.17

Place the required Reverse Insert (diameter, inclination and height) on the Reverse Tray, reproducing the configuration determined with the trial reduction. Use the marks at the highest point of inclined Reverse Inserts and the scale on offset and inclined Reverse Trays to do so.

Impact the Reverse Insert with the convex Impactor for Reverse Inserts until the gap between Insert and Tray is completely closed. The entire prosthesis is carefully impacted into the humerus until the Reverse Tray's underside rests on the bone surface.



Figure 6.18

Perform reduction and final check. If adjustments are necessary, both the Reverse Insert and the Reverse Tray can be removed. For further information on component removal, refer to chapter 7.

6.2.1.2 Cemented Humeral Standard Stem Implantation

NOTE: For cemented implantation, select the Humeral Standard Stem one or two sizes smaller than the last Compressor used. When selecting the Humeral Stem one size smaller than the last Compressor, a cement mantle thickness of approx. 0.5 mm is achieved.

NOTE: Alternatively to assembling the component in situ as described here, the component can be completely assembled on the sterile table and impacted as a whole afterwards. In this case, follow the workflow described here correspondingly.

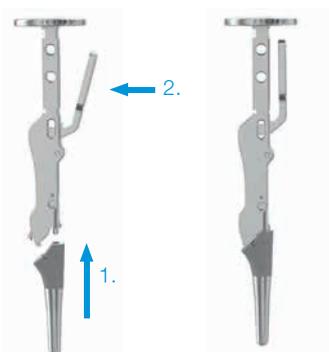


Figure 6.19

The use of high viscosity cement is recommended for cementation. Remove the transportation lock (white plastic cover) from the selected Humeral Stem. Connect the Humeral Stem to the Handle.



Figure 6.20

Clean the bone using jet or pulse lavage and apply the cement. Insert the Humeral Stem into the soft cement taking into account the desired retroversion. For this purpose, the Alignment Rod is screwed into the appropriate hole in the Handle impactation plate rim. Make sure to select the correct set of holes for left and right side treatment.



Figure 6.21

Alternatively, place the Alignment Rod Connector on the Handle and insert the Alignment Rod in the appropriate hole. Make sure to select the correct position of the Alignment Rod Connector for left and right side treatment.



Figure 6.22

Manually press down the Stem into the soft cement until it is positioned at the same level as the last Compressor used. Remove excessive bone cement. With the Handle, the prosthesis is held in position until the cement is cured.



Figure 6.23

Remove the Handle.
Assemble the Reverse Tray and Reverse Insert as described in 6.1. Perform reduction and final check. If adjustments are necessary, both the Reverse Insert and the Reverse Tray can be removed. For further information on component removal, refer to chapter 7.

7. Component Removal

All LINK Embrace components can be removed by means of specifically designed instruments.

7.1 Removal of Humeral Standard and Short Stems



Figure 7.1

For removal of Humeral Standard and Short Stems, connect the Handle for Compressors to the humeral component in situ.

Assemble the Extraction device by sliding the Slaphammer over the Stem for Slaphammer. Screw the Extraction device into the threaded hole of the Extraction Hook.



Figure 7.2

Attach the Extraction device to the Handle by sliding the two Hook bolts into the holes at the Handle.

Remove the humeral component by applying appropriate blows with the Slaphammer.

7.2 Removal of Reverse Trays



Figure 7.3

Push a small chisel into the gap between Reverse Insert and Reverse Tray and remove the Insert by circumferential levering with the chisel. To facilitate removal you may turn a Bone Screw through the PE-Insert, pushing the Insert off the Tray.



Figure 7.4

Position the tips of an appropriate instrument, e.g. a LINK Bankart Perforating Forceps (item code 64-4160/09) into the grooves of the Reverse Tray and hold the instrument firmly.



Figure 7.5

Remove the Fixation Screw within the Reverse Tray by turning it counterclockwise using the Torx 25 Screwdriverbit connected to the Ratchet



Figure 7.6

Slide the Separator Wrench into the gap between Reverse Tray and Humeral Component.

Impact the Separator Wrench with light mallet blows. Repeat this procedure at another position in case the component cannot be removed.



Figure 7.7

In case the taper connection of the components cannot be released with the Separator Wrench, apply the extraction instruments as described subsequently.

Connect the Reverse Tray Extraction Bolt to the T-Handle.

Introduce the threaded extractor tip into the Reverse Tray's central hole.



Figure 7.8

Detach the Reverse Tray from the humeral component by turning the T-Handle clockwise, holding the Forceps with your other hand as a counter torque, until the Tray is completely separated from the humeral component.

In case of revision or conversion surgery, visually check the female taper of the humeral component for integrity. Mount the required anatomic components as described in the surgical technique of the LINK Embrace Shoulder System – Anatomic Configuration.

7.3 Removal of Glenospheres



Figure 7.9

Connect the Torx 20 Screwdriverbit to the Ratchet and introduce the screwdriver tip into the head of the Glenosphere locking screw. Untighten the screw by turning the Screwdriver counterclockwise. Make sure the screw is completely loose.

Slide the Extraction Cap for Glenospheres (metal Cap) over the central rod between the branches of the Handle for Glenospheres.

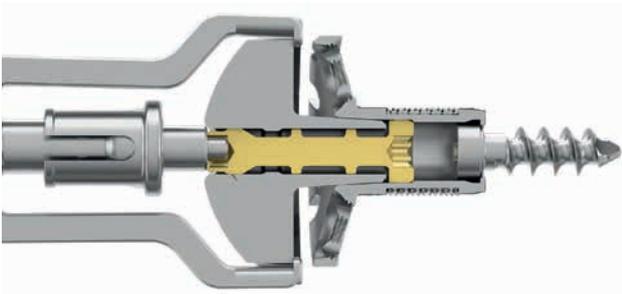


Figure 7.10

Turn the Handle knob counterclockwise in order to open the pincers. Attach the Handle to the implanted Glenosphere, inserting the metal Cap tip into the Glenosphere hole. Position the pincers in the lateral Glenosphere grooves. Turn the instrument knob clockwise to close the pincers.

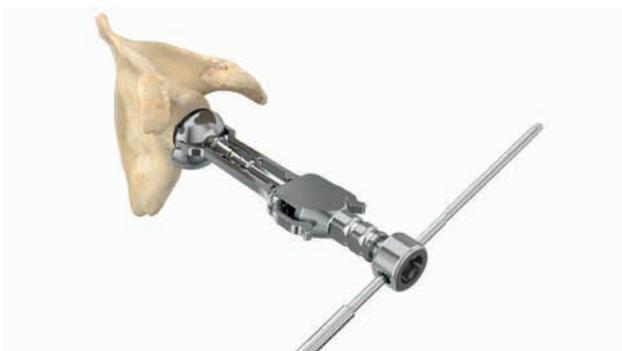


Figure 7.11

Detach the Glenosphere by continued turning the Handle knob clockwise, separating the taper connection between Glenosphere and glenoid component. To facilitate turning the knob, slide a Screwdriverbit through the knob hole and use it as a T-Handle.

Go on turning the knob clockwise until the Glenosphere is completely separated from the Reverse Baseplate.

7.4 Removal of Reverse Glenoid Baseplates



Figure 7.12

After removal of the Glenosphere, remove all peripheral Bone Screws and, if applied, the central Bone Screw using the Torx 25 Screwdriverbit connected to the Ratchet.

Screw the Extraction Adapter into the central hole of the Reverse Baseplate.



Figure 7.13

Slide the Slaphammer over the Slaphammer Stem and attach the T-Handle. Screw the assembled Slaphammer onto the Extraction Adapter.

Extract the Reverse Baseplate by carefully sliding the hammer and stabilizing the instrument with your other hand on the T-Handle.

8. Implants

Humeral Short Stems

MAT *Tibotan*-S, Fixation: cementless



REF	Length (l) mm	Diameter (d) mm	Coating/Surface
640-175/12	75	12	CaP-coating
640-175/13	75	13	CaP-coating
640-175/14	75	14	CaP-coating
640-175/15	75	15	CaP-coating
640-175/16	75	16	CaP-coating
640-175/17	75	17	CaP-coating
640-175/18	75	18	CaP-coating
640-175/19	75	19	CaP-coating
640-175/20	75	20	CaP-coating

Humeral Standard Stems

MAT *Tibotan*-S, Fixation: cemented/cementless



REF	Length (l) mm	Diameter (d) mm	Coating/Surface
640-100/12	100	12	-
640-100/13	100	13	-
640-100/14	100	14	-
640-100/15	100	15	-
640-100/16	100	16	-
640-100/17	100	17	-
640-100/18	100	18	-
640-100/19	100	19	-
640-100/20	100	20	-
640-100/21	100	21	-
640-100/22	100	22	-
640-100/23	100	23	-
640-100/24	100	24	-

Humeral Standard Stems


MAT *Ti/otan*-S, Fixation: cementless



REF	Length (l) mm	Diameter (d) mm	Coating/Surface
640-110/12	100	12	CaP-coating
640-110/13	100	13	CaP-coating
640-110/14	100	14	CaP-coating
640-110/15	100	15	CaP-coating
640-110/16	100	16	CaP-coating
640-110/17	100	17	CaP-coating
640-110/18	100	18	CaP-coating
640-110/19	100	19	CaP-coating
640-110/20	100	20	CaP-coating
640-110/21	100	21	CaP-coating
640-110/22	100	22	CaP-coating
640-110/23	100	23	CaP-coating
640-110/24	100	24	CaP-coating

Reverse Glenoid Baseplates

MAT *Ti/otan*-E

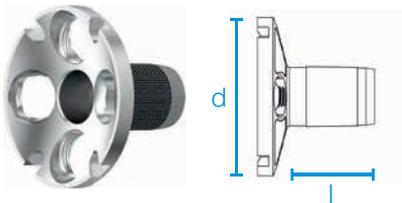

REF	Diameter (d) mm	Length (l) mm	Coating/Surface
645-080/20	28	15	TrabecuLink
645-080/30	28	25	TrabecuLink

Cortical Bone Screws

MAT *Ti60tan*-S, Torx 25



REF	Diameter (mm)	Length (mm)
645-073/20	4.5	20
645-073/25	4.5	25
645-073/30	4.5	30
645-073/35	4.5	35
645-073/40	4.5	40
645-073/50	4.5	50
645-073/60	4.5	60

Cortical Bone Screws - angle-stable

MAT *Ti60tan*-S, Torx 25



REF	Diameter (mm)	Length (mm)
645-075/20	4.5	20
645-075/25	4.5	25
645-075/30	4.5	30
645-075/35	4.5	35
645-075/40	4.5	40
645-075/50	4.5	50
645-075/60	4.5	60

Central Cancellous Bone Screws

MAT *Ti60tan*-S, Torx 25



REF	Diameter (mm)	Length (mm)
645-077/20	6.0	20
645-077/25	6.0	25
645-077/30	6.0	30

Cancellous Bone Screws

MAT *Ti60tan*-S, Torx 25



REF	Diameter (mm)	Length (mm)
645-070/20	6.0	20
645-070/25	6.0	25
645-070/30	6.0	30
645-070/35	6.0	35
645-070/40	6.0	40
645-070/50	6.0	50
645-070/60	6.0	60

Humeral Reverse Tray - neutral

MAT EndoDur-S (CoCrMo), Fixation Screw included (*Ti*tan-S)



REF	Material	Coating/Surface
643-010/00	EndoDur-S	-

Humeral Reverse Tray - 3 mm offset

MAT EndoDur-S (CoCrMo), Fixation Screw included (*Ti*tan-S)



REF	Material	Coating/Surface
643-010/03	EndoDur-S	-

Humeral Reverse Tray - inclined 10°

MAT EndoDur-S (CoCrMo), Fixation Screw included (*Ti*tan-S)



REF	Material	Coating/Surface
643-020/10	EndoDur-S	-

Reverse Inserts

MAT UHMWPE



REF	Height (mm)	Diameter (mm)	Material
643-036/00	0	36	UHMWPE
643-036/03	3	36	UHMWPE
643-036/06	6	36	UHMWPE
643-039/00	0	39	UHMWPE
643-039/03	3	39	UHMWPE
643-039/06	6	39	UHMWPE
643-042/00	0	42	UHMWPE
643-042/03	3	42	UHMWPE
643-042/06	6	42	UHMWPE
643-236/00	0	36	UHMWPE/E-DUR
643-236/03	3	36	UHMWPE/E-DUR
643-236/06	6	36	UHMWPE/E-DUR
643-239/00	0	39	UHMWPE/E-DUR
643-239/03	3	39	UHMWPE/E-DUR
643-239/06	6	39	UHMWPE/E-DUR
643-242/00	0	42	UHMWPE/E-DUR
643-242/03	3	42	UHMWPE/E-DUR
643-242/06	6	42	UHMWPE/E-DUR

Reverse Inserts - inclined 10°

MAT UHMWPE



REF	Height (mm)	Diameter (mm)	Material
643-036/10	0	36	UHMWPE
643-036/13	3	36	UHMWPE
643-036/16	6	36	UHMWPE
643-039/10	0	39	UHMWPE
643-039/13	3	39	UHMWPE
643-039/16	6	39	UHMWPE
643-042/10	0	42	UHMWPE
643-042/13	3	42	UHMWPE
643-042/16	6	42	UHMWPE
643-236/10	0	36	UHMWPE/E-DUR
643-236/13	3	36	UHMWPE/E-DUR
643-236/16	6	36	UHMWPE/E-DUR
643-239/10	0	39	UHMWPE/E-DUR
643-239/13	3	39	UHMWPE/E-DUR
643-239/16	6	39	UHMWPE/E-DUR
643-242/10	0	42	UHMWPE/E-DUR
643-242/13	3	42	UHMWPE/E-DUR
643-242/16	6	42	UHMWPE/E-DUR

Reverse Inserts - inclined 20°

MAT UHMWPE



REF	Height (mm)	Diameter (mm)	Material
643-036/20	0	36	UHMWPE
643-036/23	3	36	UHMWPE
643-036/26	6	36	UHMWPE
643-039/20	0	39	UHMWPE
643-039/23	3	39	UHMWPE
643-039/26	6	39	UHMWPE
643-042/20	0	42	UHMWPE
643-042/23	3	42	UHMWPE
643-042/26	6	42	UHMWPE
643-236/20	0	36	UHMWPE/E-DUR
643-236/23	3	36	UHMWPE/E-DUR
643-236/26	6	36	UHMWPE/E-DUR
643-239/20	0	39	UHMWPE/E-DUR
643-239/23	3	39	UHMWPE/E-DUR
643-239/26	6	39	UHMWPE/E-DUR
643-242/20	0	42	UHMWPE/E-DUR
643-242/23	3	42	UHMWPE/E-DUR
643-242/26	6	42	UHMWPE/E-DUR

Glenospheres - neutral

MAT EndoDur-S (CoCrMo), with locking screw (EndoDur + TiNbN)



REF	Diameter (mm)	Material	Coating/Surface
646-036/00	36	EndoDur-S	-
646-039/00	39	EndoDur-S	-
646-042/00	42	EndoDur-S	-

Glenospheres - eccentric


MAT EndoDur-S (CoCrMo), with locking screw (EndoDur + TiNbN)




REF	Diameter (mm)	Eccentricity (mm)	Material	Coating/Surface
646-036/03	36	3.0	EndoDur-S	-
646-039/03	39	3.5	EndoDur-S	-
646-042/03	42	4.0	EndoDur-S	-

9. Instruments

650-001/00 General Set

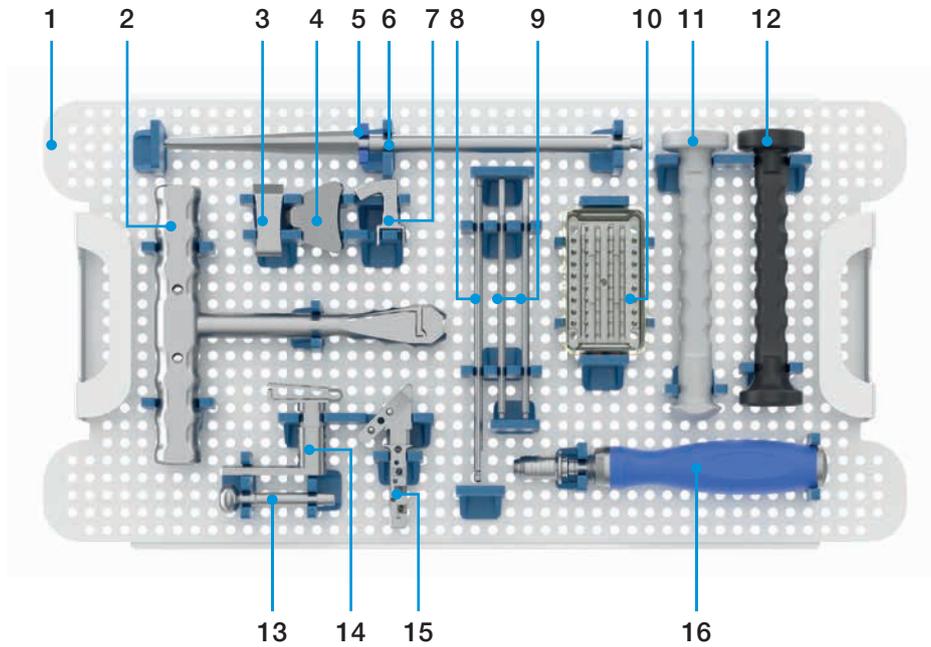


1	650-011/00	General Set Tray
2	15-6053/00	T-Handle (Hudson fitting)
3	632-005/02	Resection Block (for Delto-Pectoral Approach)
4	632-005/07	Resection Block (for Lateral Approach)
5	630-001/11	Depth Stop Disk
6	630-001/10	Starter Awl
7	632-005/09	Alignment Rod Connector
8	630-001/06	Screwdriverbit (T25, for Bone Screws)
9	632-005/08 × 2	Alignment Rod
10	319-601/30	Sterilizing Box, contains:
	632-005/65 × 4	Fixation Pin
11	643-001/01	Impactor (for Reverse Inserts and PE Glenoids)
12	632-001/01	Impactor (for Humeral Heads)
13	632-005/01	Resection Guide Connector
14	632-005/00	Resection Guide (for Humeral Head)
15	632-005/10	Extramedullary Resection Guide
16	134-220/03	Torque Wrench, 3 Nm (AO fitting)

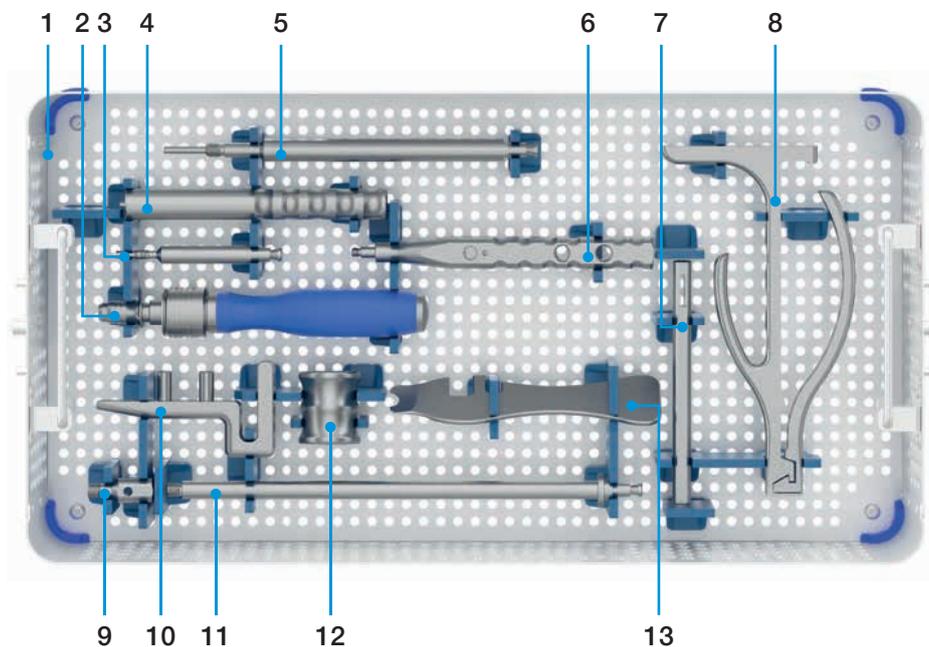


1	650-011/00	General Set Tray
2	80-2014	Ratchet Handle (AO fitting)
3	645-090/13	Reverse Tray Extraction Bolt
4	645-090/11	Counter Sleeve (for Head Adapter Extraction Bolt)
5	645-090/09	Head Adapter Extraction Bolt
6	631-001/01	Impactor (for Modular Stems)
7	445-121/00	Pin Inserter, universal
8	445-120/00	Pin Inserter/Extractor, universal
9	645-090/07	Extraction Adapter (for Convertible Metal-Back and Reverse Baseplate)
10	645-090/01	Extraction Hook
11	645-090/03	Stem for Slaphammer
12	645-090/05	Slaphammer
13	645-090/21	Separator Wrench

650-003/00 Short & Standard Stem Set

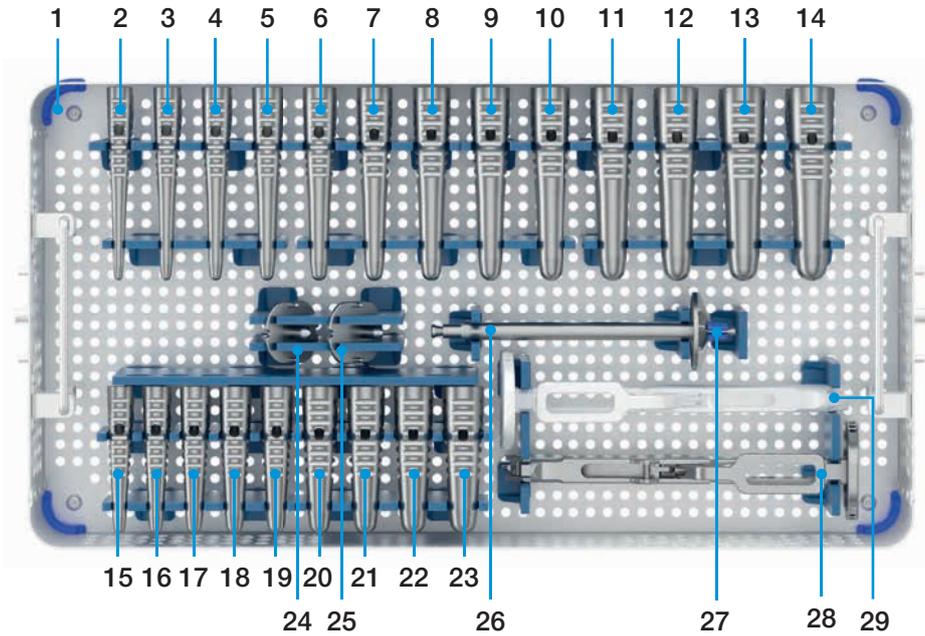

1	650-013/00	Short & Standard Stem Set Tray
2	630-100/12	Compressor (for Humeral Standard Stems), Ø 12
3	630-100/13	Compressor (for Humeral Standard Stems), Ø 13
4	630-100/14	Compressor (for Humeral Standard Stems), Ø 14
5	630-100/15	Compressor (for Humeral Standard Stems), Ø 15
6	630-100/16	Compressor (for Humeral Standard Stems), Ø 16
7	630-100/17	Compressor (for Humeral Standard Stems), Ø 17
8	630-100/18	Compressor (for Humeral Standard Stems), Ø 18
9	630-100/19	Compressor (for Humeral Standard Stems), Ø 19
10	630-100/20	Compressor (for Humeral Standard Stems), Ø 20
11	630-100/21	Compressor (for Humeral Standard Stems), Ø 21
12	630-100/22	Compressor (for Humeral Standard Stems), Ø 22
13	630-100/23	Compressor (for Humeral Standard Stems), Ø 23
14	630-100/24	Compressor (for Humeral Standard Stems), Ø 24
15	630-075/12	Compressor (for Humeral Short Stems), Ø 12
16	630-075/13	Compressor (for Humeral Short Stems), Ø 13
17	630-075/14	Compressor (for Humeral Short Stems), Ø 14
18	630-075/15	Compressor (for Humeral Short Stems), Ø 15
19	630-075/16	Compressor (for Humeral Short Stems), Ø 16
20	630-075/17	Compressor (for Humeral Short Stems), Ø 17
21	630-075/18	Compressor (for Humeral Short Stems), Ø 18
22	630-075/19	Compressor (for Humeral Short Stems), Ø 19
23	630-075/20	Compressor (for Humeral Short Stems), Ø 20
24	630-001/14	Humerus Protection Plate, 6 mm Offset
25	630-001/15	Humerus Protection Plate, neutral
26	630-001/07	Finishing Reamer
27	630-001/09	Sleeve (for Finishing Reamer)
28	630-001/01	Handle (for Compressors and Proximal Bodies)
29	630-001/01	Handle (for Compressors and Proximal Bodies, on request)


650-005/00 Glenoid Set

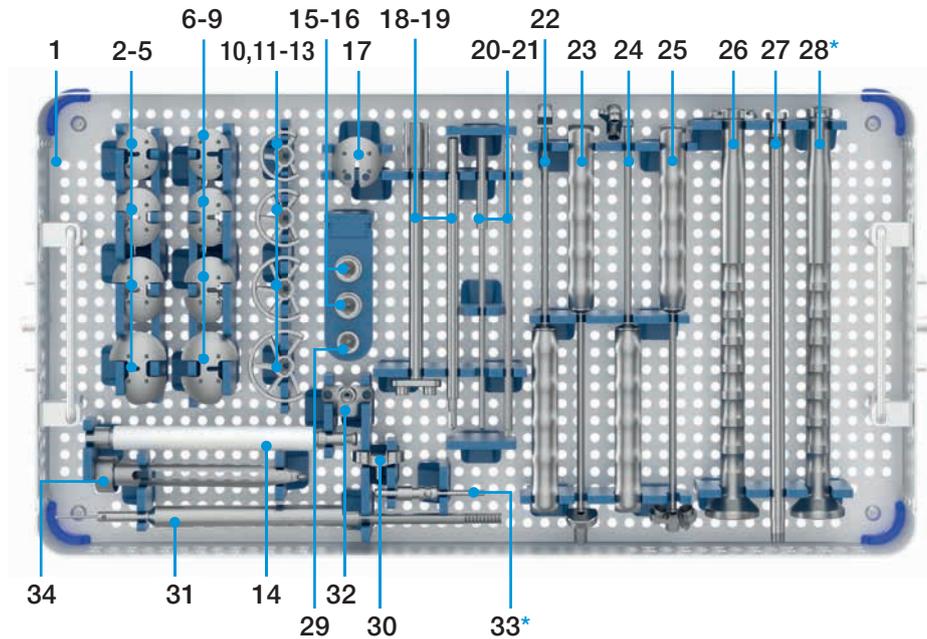

1	650-015/00	Glenoid Set Tray
2	645-001/09	Glenoid Sizer, left, small
3	645-001/11	Glenoid Sizer, left, medium
4	645-001/13	Glenoid Sizer, left, large
5	645-001/15	Glenoid Sizer, left, x-large
6	645-001/10	Glenoid Sizer, right, small
7	645-001/12	Glenoid Sizer, right, medium
8	645-001/14	Glenoid Sizer, right, large
9	645-001/16	Glenoid Sizer, right, x-large
10	645-001/28	Glenoid Reamer, small (Ø 28)
11	645-001/32	Glenoid Reamer, medium (Ø 32)
12	645-001/36	Glenoid Reamer, large (Ø 36)
13	645-001/40	Glenoid Reamer, x-large (Ø 40)
14	645-001/01	Drive Shaft (for Glenoid Preparation, cannulated, Hudson fitting)
15	645-002/03	Drill, standard (for Reverse Glen. Baseplate for Central Peg)
16	645-002/05	Drill, long (for Reverse Glenoid Baseplate, for Central Peg)
17	645-002/28	K-Wire Positioner for Reverse Baseplate
18	645-002/12	Guide Handle (for K-Wire)
19	645-002/07	Drill (for Glenoids, for Peripheral Pegs)
20	64-8022	Twist Drill, Ø 3.2
21	80-2030	Screwdriverbit (T20, for Glenospheres)
22	645-080/50	Handle (for Glenoid Sizers and Drill Templates)
23	645-080/60	Drill Guide (for Central Screws)
24	645-080/52	Drill Guide A/P monoaxial
25	645-080/54	Drill Guide "S/I" polyaxial
26	645-080/56	Impactor (for Reverse Baseplate)
27	645-080/59	Shaft for Impactor (for Reverse Baseplate)
28	645-080/58*	Impactor (for Convertible Metal-Back)
29	645-002/01	Drill (for Cemented All Poly Glenoids, for Central Peg)
30	645-002/09	Drill Template (for Cemented All Poly Glenoids, for Peripheral Pegs)
31	645-080/64	Depth Gauge (for Bone Screws)
32	645-003/09	Drill Template (for Convertible Metal-Back*, for Peripheral Pegs)
33	645-002/08*	Fixation Pin (for Drill Templates)
34	645-002/15	Repositioner (for K-Wire)

* not available in the US

650-007/00 Reverse Set

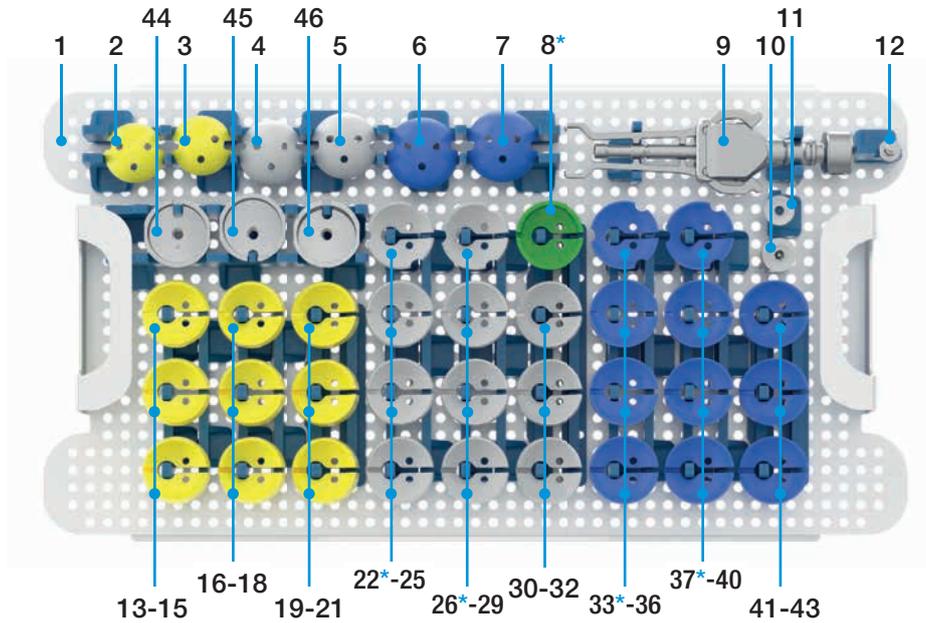


1	650-017/00	Reverse Set Tray
2	646-536/03	Trial Glenosphere, Ø 36, eccentric
3	646-536/00	Trial Glenosphere, Ø 36, neutral
4	646-539/03	Trial Glenosphere, Ø 39, eccentric
5	646-539/00	Trial Glenosphere, Ø 39, neutral
6	646-542/03	Trial Glenosphere, Ø 42, eccentric
7	646-542/00	Trial Glenosphere, Ø 42, neutral
8	643-930/09*	Humeral Trial Extender
9	646-530/00	Handle for Glenospheres
10	646-530/04	Cap (for eccentric Glenospheres)
11	646-530/02	Cap (for neutral Glenospheres)
12	645-090/23	Extraction Cap (for Glenosphere Removal)
13	643-836/00	Reverse Trial Insert, Ø 36, H0 mm
14	643-836/03	Reverse Trial Insert, Ø 36, H3 mm
15	643-836/06	Reverse Trial Insert, Ø 36, H6 mm
16	643-836/10	Reverse Trial Insert, Ø 36, H0 mm, 10°
17	643-836/13	Reverse Trial Insert, Ø 36, H3 mm, 10°
18	643-836/16	Reverse Trial Insert, Ø 36, H6 mm, 10°
19	643-836/20	Reverse Trial Insert, Ø 36, H0 mm, 20°
20	643-836/23	Reverse Trial Insert, Ø 36, H3 mm, 20°
21	643-836/26	Reverse Trial Insert, Ø 36, H6 mm, 20°
22	643-839/33*	Reverse Trial Insert, Ø 39, H-3 mm
23	643-839/00	Reverse Trial Insert, Ø 39, H0 mm
24	643-839/03	Reverse Trial Insert, Ø 39, H3 mm
25	643-839/06	Reverse Trial Insert, Ø 39, H6 mm
26	643-839/43*	Reverse Trial Insert, Ø 39, H-3 mm, 10°
27	643-839/10	Reverse Trial Insert, Ø 39, H0 mm, 10°
28	643-839/13	Reverse Trial Insert, Ø 39, H3 mm, 10°
29	643-839/16	Reverse Trial Insert, Ø 39, H6 mm, 10°

Continue on next page >

* not available in the US

30	643-839/20	Reverse Trial Insert, Ø 39, H0 mm, 20°
31	643-839/23	Reverse Trial Insert, Ø 39, H3 mm, 20°
32	643-839/26	Reverse Trial Insert, Ø 39, H6 mm, 20°
33	643-842/33*	Reverse Trial Insert, Ø 42, H-3 mm
34	643-842/00	Reverse Trial Insert, Ø 42, H0 mm
35	643-842/03	Reverse Trial Insert, Ø 42, H3 mm
36	643-842/06	Reverse Trial Insert, Ø 42, H6 mm
37	643-842/43*	Reverse Trial Insert, Ø 42, H-3 mm, 10°
38	643-842/10	Reverse Trial Insert, Ø 42, H0 mm, 10°
39	643-842/13	Reverse Trial Insert, Ø 42, H3 mm, 10°
40	643-842/16	Reverse Trial Insert, Ø 42, H6 mm, 10°
41	643-842/20	Reverse Trial Insert, Ø 42, H0 mm, 20°
42	643-842/23	Reverse Trial Insert, Ø 42, H3 mm, 20°
43	643-842/26	Reverse Trial Insert, Ø 42, H6 mm, 20°
44	643-910/00	Reverse Trial Tray (neutral)
45	643-910/03	Reverse Trial Tray (3 mm offset)
46	643-920/10	Reverse Trial Tray (10° inclined)

* not available in the US

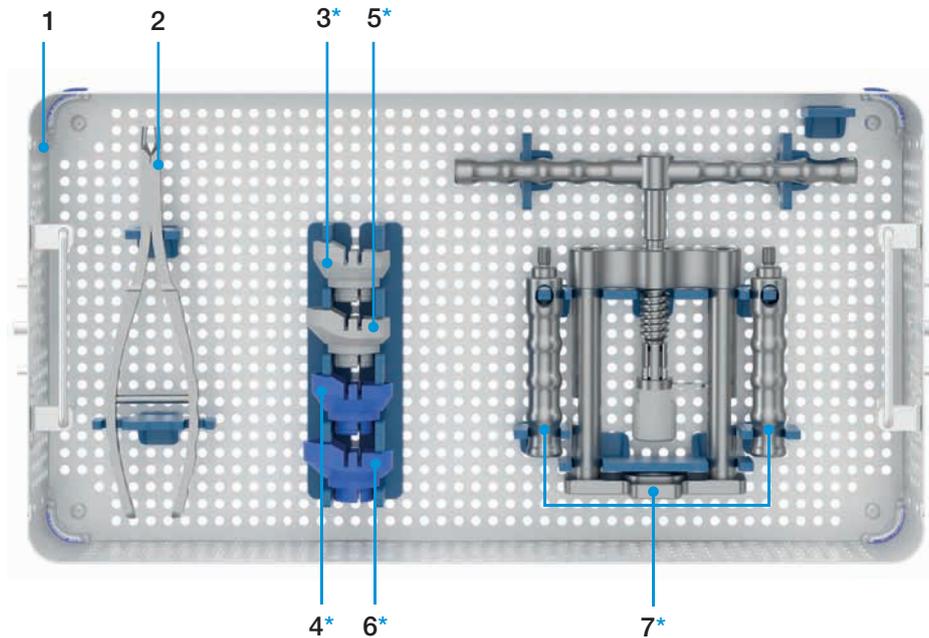

1	650-017/00	Reverse Set Tray
2	15-2042	Insertion Forceps
3	646-530/16*	Support for Press, Ø 39, eccentric
4	646-530/18*	Support for Press, Ø 42, eccentric
5	646-530/15*	Support for Press, Ø 39, neutral
6	646-530/17*	Support for Press, Ø 42, neutral
7	646-530/11*	Press

* not available in the US

10. X-ray Templates

1	650-030/01	Humeral Short & Humeral Standard Stems
2	650-030/05	Reverse Trays & Reverse Inserts & Humeral Extender
3	650-030/06	Reverse Glenoid Baseplates & Glenospheres

11. System Compatibility

This chapter comprises all tables showing component compatibility and restrictions within the LINK Embrace Shoulder system. For further information refer to the specified chapter.

Reverse Inserts: Types and Allowed Combinations

Chapter 6 Reverse Humeral Component Trialing

Reverse Humeral Inserts		
Diameter	Inclination	Heights
		UHMWPE
36	0°	0, 3, 6
	10°	0, 3, 6
	20°	0, 3, 6
39	0°	0, 3, 6
	10°	0, 3, 6
	20°	0, 3, 6
42	0°	0, 3, 6
	10°	0, 3, 6
	20°	0, 3, 6
to be combined with Glenospheres made of:		EndoDur

Table 6.1: Reverse Inserts: types and allowed combinations. Numerical data in mm unless otherwise noted.

Please note the following regarding the use of our implants:

1. Choosing the right implant is very important.

The size and shape of the human bone determines the size and shape of the implant and also limits the load capacity.

Implants are not designed to withstand unlimited physical stress. Demands should not exceed normal functional loads.

2. Correct handling of the implant is very important.

Under no circumstances should the shape of a finished implant be altered, as this shortens its life span. Our implants must not be combined with implants from other manufacturers. The instruments indicated in the Surgical Technique must be used to ensure safe implantation of the components.

3. Implants must not be reused.

Implants are supplied sterile and are intended for single use only. Used implants must not be used again.

4. After-treatment is also very important.

The patient must be informed of the limitations of the implant. The load capacity of an implant cannot compare with that of healthy bone!

5. Unless otherwise indicated, implants are supplied in sterile packaging.

Note the following conditions for storage of packaged implants:

- Avoid extreme or sudden changes in temperature.
- Sterile implants in their original, intact protective packaging may be stored in permanent buildings up until the "Use by" date indicated on the packaging.
- They must not be exposed to frost, dampness or direct sunlight, or mechanical damage.
- Implants may be stored in their original packaging for up to 5 years after the date of manufacture. The "Use by" date is indicated on the product label.
- Do not use an implant if the packaging is damaged.

6. Traceability is important.

Please use the documentation stickers provided to ensure traceability.

7. Further information on the material composition is available on request from the manufacturer.

Follow the instructions for use!

Waldemar Link GmbH & Co. KG, Hamburg

All content in this catalog, including text, pictures and data, is protected by law. Every instance of use, whether in part or in whole and which is not permitted by law, is subject to our prior consent. In particular, this applies to the reproduction, editing, translation, publishing, saving, processing, or passing on of content stored in databases or other electronic media and systems, in any manner or form. The information in the catalogs is solely intended to describe the products and does not constitute a guarantee. The Surgical Technique described has been written to the best of our knowledge and belief, but it does not relieve the surgeon of his/her responsibility to duly consider the particularities of each individual case.

Products shown in this document may not be available in your country. The product availability is subject to the approval and/or registration regulations of the respective country. Please contact Waldemar Link GmbH & Co. KG if you have questions about the availability of LINK products in your country.

Waldemar Link GmbH & Co. KG and/or other corporate affiliated entities own, use or have applied for the following trademarks in many jurisdictions: LINK, BiMobile, SP II, Modell Lubinus, E-Dur, EndoDur, T.O.P. II, BetaCup, CombiCup PF, CombiCup SC, CombiCup R, MobileLink, C.F.P., LCU, SP-CL, LCP, MIT-H, Endo-Model, Endo-ModelSL, MP, MEGASYSTEM-C, GEMINI SL, SPAR-K, LCK, Link OptiStem, HX, TiCaP, X-LINKed, PorAg, LINK PorEx, BiPorEx, PorEx-Z, TrabecuLink, Tilastan, customLINK, RescueSleeve, Stactip, VACUCAST.

Other trademarks and trade names may be used in this document to refer to either the entities claiming the marks and/or names or their products and are the property of their respective owners.

This publication is intended for distribution in the US only.